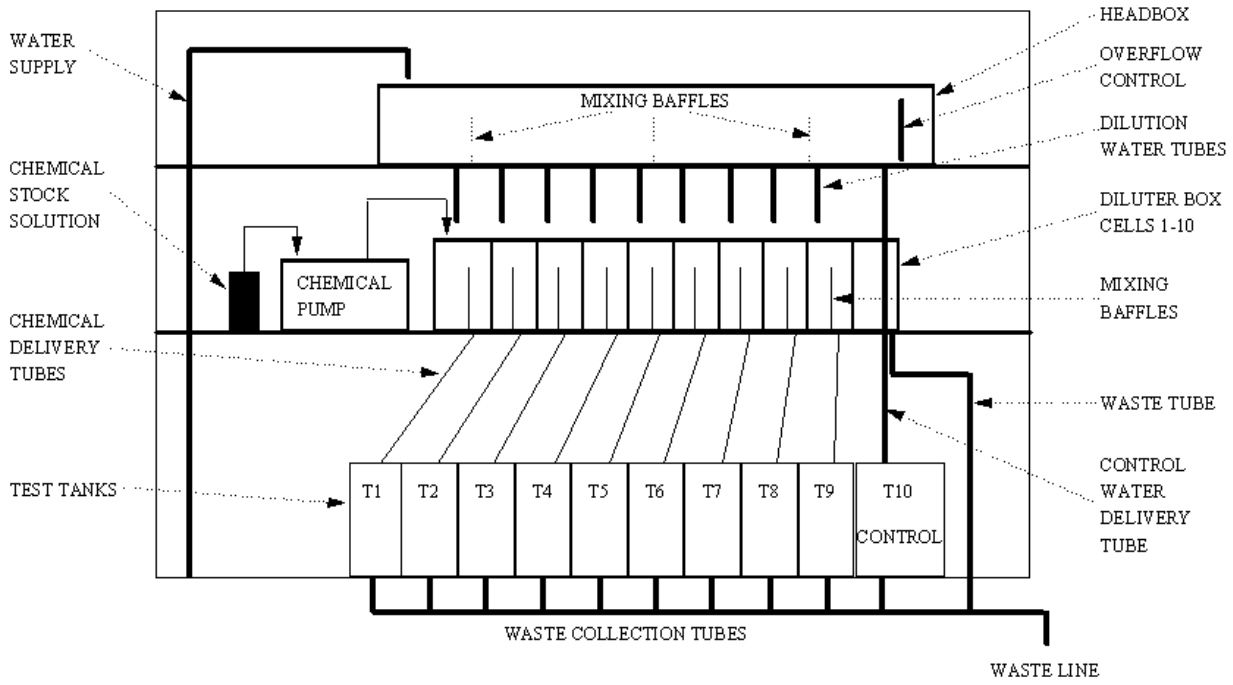Attachment 2
Diagram of continuous-flow toxicity test system